



For Research Use Only, Not for use in diagnostic procedures

ELISA Kit for Measuring Human LYPD6B

CircuLex Human LYPD6B ELISA Kit

Cat# CY-8212

Intended Use.....	1
Storage.....	1
Introduction.....	2
Principle of the Assay.....	3
Materials Provided.....	4
Materials Required but not Provided.....	4
Precautions and Recommendations.....	5
Sample Collection and Storage.....	6
Detailed Protocol.....	7-9
Calculations.....	10
Measurement Range.....	10
Troubleshooting.....	10
Reagent Stability.....	10
Assay Characteristics.....	11-13
Example of Test Results.....	14
References.....	15
Related Products.....	15

Intended Use

The MBL Research Product **CircuLex Human LYPD6B ELISA Kit** is used for the quantitative measurement of human LYPD6B in serum, plasma, and cell culture supernatant.

Individual users should determine appropriate conditions when using other types of samples.

This assay kit is for research use only and not for use in diagnostic or therapeutic procedures.

Storage

- Upon receipt store all components at 4°C.
- Do not expose reagents to excessive light.


Introduction

LYPD6B (Ly6/PLAUR domain-containing protein 6B), a member of Ly-6 superfamily, is isolated from human testis cDNA library (1,2). Ly-6 (lymphocyte antigen 6) superfamily members are cysteine-rich, normally GPI (glycosyl phosphatidylinositol)-anchored cell surface proteins, which have definite or putative immune related roles (3,4). LYPD6B contains signal peptide (N-terminal), UPAR/Ly6 domain, propeptide (C-terminal) and mature human LYPD6B is 125 amino acids in length and especially highly expressed in testis, lung, stomach, and prostate and localized in the cytoplasm. LYPD6B overexpressed in HEK 293T cells is able to activate the transcriptional activities of AP1 (PMA), but a reason of this event is unclear (1).

Principle of the Assay

The MBL Research Product **CircuLex Human LYPD6B ELISA Kit** employs the quantitative sandwich enzyme immunoassay technique. An antibody specific for human LYPD6B is pre-coated onto a microplate. Standards and samples are pipetted into the wells and the immobilized antibody binds any human LYPD6B present. After washing away any unbound substances, a biotinylated monoclonal antibody specific for human LYPD6B is added to the wells. Following a wash to remove any unbound biotinylated antibody, Streptavidin-HRP is added to the wells. After washing away any unbound Streptavidin-HRP, HRP remaining on the well is allowed to react with the substrate H₂O₂-tetramethylbenzidine. The reaction is stopped by addition of acidic solution and absorbance of the resulting yellow product is measured at 450 nm. The absorbance is proportional to the concentration of human LYPD6B. A standard curve is constructed by plotting absorbance values versus human LYPD6B concentrations of calibrators, and concentrations of unknown samples are determined using this standard curve.

Summary of Procedure

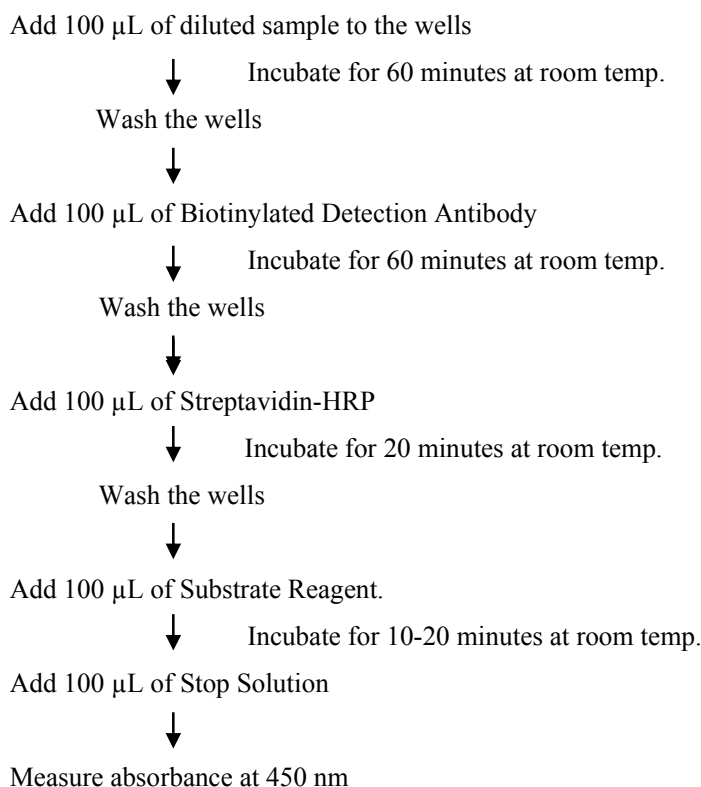

Materials Provided

All samples and standards should be assayed in duplicate. The following components are supplied and are sufficient for the one 96-well microplate kit.

Microplate: One microplate supplied ready to use, with 96 wells (12 strips of 8-wells) in a foil, zip-lock bag with a desiccant pack. Wells are pre-coated with anti-human LYPD6B monoclonal antibody as a capture antibody.

10X Wash Buffer: One bottle containing 100 mL of 10X buffer containing Tween®-20.

Sample Dilution Buffer: One bottle containing 50 mL of 1X buffer; use for standard and sample dilution. Ready to use.

Human LYPD6B Standard: One vial containing X* ng of lyophilized recombinant human LYPD6B.

***The amount is changed depending on lot. See the real "User's Manual" included in the kit box.**

Biotinylated Detection Antibody: One vial containing 12 mL of biotinylated anti-human LYPD6B monoclonal antibody. Ready to use.

100X Streptavidin-HRP: One vial containing 120 µL of 100X HRP (horseradish peroxidase) conjugated streptavidin.

Streptavidin-HRP Dilution Buffer: One bottle containing 12 mL of 1X buffer; use for dilution of 100X Streptavidin-HRP.

Substrate Reagent: One bottle containing 20 mL of the chromogenic substrate, tetra-methylbenzidine (TMB). Ready to use.

Stop Solution: One bottle containing 20 mL of 1 N H₂SO₄. Ready to use.

Materials Required but not Provided

- **Pipettors:** 2-20 µL, 20-200 µL and 200-1,000 µL precision pipettors with disposable tips.
- **Precision repeating pipettor**
- **Orbital microplate shaker**
- **Microcentrifuge and tubes** for sample preparation.
- **Vortex mixer**
- **(Optional) Microplate washer:** Manual washing is possible but not preferable.
- **Plate reader** capable of measuring absorbance in 96-well plates at dual wavelengths of 450 nm/540 nm. Dual wavelengths of 450/550 or 450/595 nm can also be used. The plate can also be read at a single wavelength of 450 nm, which will give a somewhat higher reading.
- **(Optional) Software package facilitating data generation and analysis**
- **500 or 1,000 mL graduated cylinder.**
- **Reagent reservoirs**
- **Deionized water of the highest quality**
- **Disposable paper towels**

Precautions and Recommendations

- **Although we suggest to conduct experiments as outlined below, the optimal experimental conditions will vary depending on the parameters being investigated, and must be determined by the individual user.**
- Allow all the components to come to room temperature before use.
- All microplate strips that are not immediately required should be returned to the zip-lock pouch, which must be carefully resealed to avoid moisture absorption.
- Do not use kit components beyond the indicated kit expiration date.
- Use only the microtiter wells provided with the kit.
- Rinse all detergent residue from glassware.
- Use deionized water of the highest quality.
- Do not mix reagents from different kits.
- The buffers and reagents in this kit may contain preservatives or other chemicals. Care should be taken to avoid direct contact with these reagents.
- Do not mouth pipette or ingest any of the reagents.
- Do not smoke, eat, or drink when performing the assay or in areas where samples or reagents are handled.
- Dispose of tetra-methylbenzidine (TMB) containing solutions in compliance with local regulations.
- Avoid contact with Substrate Solution which contains hydrogen peroxide.
- **CAUTION: Biological samples may be contaminated with infectious agents. Do not ingest, expose to open wounds or breathe aerosols. Wear protective gloves and dispose of biological samples properly.**
- **CAUTION: Stop Solution is a strong acid. Wear disposable gloves and eye protection when handling the solution.**

Sample Collection and Storage

Serum: Use a serum separator tube and allow samples to clot for 60 ± 30 minutes. Centrifuge the samples at 4°C for 10 minutes at $1,000 \times g$. Remove serum and assay immediately or store samples on ice for up to 6 hours before assaying. Aliquots of serum may also be stored at below -70°C for extended periods of time. Avoid repeated freeze-thaw cycles.

Plasma: Collect plasma using EDTA-2Na as the anticoagulant. If possible, collect the plasma into a mixture of EDTA-2Na and Futhan5 to stabilize the sample against spontaneous *in vitro* complement activation. Immediately centrifuge samples at 4°C for 15 minutes at $1,000 \times g$. Assay immediately or store samples on ice for up to 6 hours before assaying. Aliquots of plasma may also be stored at below -70°C for extended periods of time. Avoid repeated freeze-thaw cycles.

Note: Heparin and Citrate plasma has not been validated for use in this assay.

Cell culture supernatant: Remove any particulates by centrifugation and assay immediately or aliquot and store samples at below -70°C . Avoid repeated freeze-thaw cycles.

Detailed Protocol

The MBL Research Product **CircuLex Human LYPD6B ELISA Kit** is provided with removable strips of wells so the assay can be carried out on separate occasions using only the number of strips required for the particular determination. Since experimental conditions may vary, an aliquot of the standard within the kit should be included in each assay as a calibrator. Disposable pipette tips and reagent troughs should be used for all liquid transfers to avoid cross-contamination of reagents or samples.

Preparation of Working Solutions

All reagents need to be brought to room temperature prior to the assay. Assay reagents are supplied ready-to-use, with the exception of **10X Wash Buffer**, **100X Streptavidin-HRP**, and **Human LYPD6B Standard**.

1. Prepare a working solution of **Wash Buffer** by adding **100 mL** of **10X Wash Buffer** to **900 mL** of deionized (distilled) water (**ddH₂O**). Mix well. Store at 4°C for two weeks or -20°C for long-term storage.
2. Prepare **1X Streptavidin-HRP** by 100-fold diluting **100X Streptavidin-HRP** with **Streptavidin-HRP Dilution Buffer** at the time of use and discard any unused portion after use.
3. Reconstitute **Human LYPD6B Standard** with **X* µL** of **ddH₂O** by gently mixing. After reconstitution, immediately dispense it in small aliquots (e.g. 100 µL) to plastic micro-centrifuge tubes and store below -70°C to avoid non-specific adsorption to glass surface and multiple freeze-thaw cycles. The concentration of human LYPD6B in vial should be **9.6 ng/mL**, which is referred to as the **Master Standard** of human LYPD6B.

***The amount is changed depending on lot. See the real "User's Manual" included in the kit box.**

Prepare Standard Solutions as follows:

Use the **Master Standard** to produce a dilution series (below). Mix each tube thoroughly before the next transfer. **Std.1 (960 pg/mL)** serves as the highest standard. **Sample Dilution Buffer** serves as the zero standard (Blank).

	Volume of Standard	Sample Dilution Buffer	Concentration
Std.1	60 µL of Master Standard (9.6 ng/mL)	540 µL	960 pg/mL
Std.2	300 µL of Std. 1 (960 pg/mL)	300 µL	480 pg/mL
Std.3	300 µL of Std. 2 (480 pg/mL)	300 µL	240 pg/mL
Std.4	300 µL of Std. 3 (240 pg/mL)	300 µL	120 pg/mL
Std.5	300 µL of Std. 4 (120 pg/mL)	300 µL	60 pg/mL
Std.6	300 µL of Std. 5 (60 pg/mL)	300 µL	30 pg/mL
Std.7	300 µL of Std. 6 (30 pg/mL)	300 µL	15 pg/mL
Blank	-	300 µL	0 pg/mL

Note: Do not use a Repeating pipette. Change tips for every dilution. Wet tip with Sample Dilution Buffer before dispensing.

Sample Preparation

Dilute samples with **Sample Dilution Buffer**.

- Serum and plasma samples may require a 50-fold dilution.
- Cell culture supernatants require appropriate dilutions.

Assay Procedure

1. Remove the appropriate number of microtiter wells from the foil pouch and place them into the well holder. Return any unused wells to the foil pouch, refold, seal with tape and store at 4°C.
2. Dilute samples with **Sample Dilution Buffer**. (See "Sample Preparation" above.)
3. Pipette **100 µL** of **Standard Solutions (Std1-Std7, Blank)** and **diluted samples** in duplicates, into the appropriate wells.
4. Incubate the plate **at room temperature (ca.25°C) for 60 minutes, shaking at ca. 300 rpm on an orbital microplate shaker.**
5. Wash 4-times by filling each well with Wash Buffer (350 µL) using a squirt bottle, multi-channel pipette, manifold dispenser or microplate washer.
6. Add **100 µL** of **Biotinylated Detection Antibody** into each well.
7. Incubate the plate **at room temperature (ca.25°C) for 60 minutes, shaking at ca. 300 rpm on an orbital microplate shaker.**
8. Wash 4-times by filling each well with Wash Buffer (350 µL) using a squirt bottle, multi-channel pipette, manifold dispenser or microplate washer.
9. Add **100 µL** of **1X Streptavidin-HRP** into each well.
10. Incubate the plate **at room temperature (ca.25°C) for 20 minutes, shaking at ca. 300 rpm on an orbital microplate shaker.**
11. Wash 4-times by filling each well with Wash Buffer (350 µL) using a squirt bottle, multi-channel pipette, manifold dispenser or microplate washer.
12. Add **100 µL** of **Substrate Reagent**. Avoid exposing the microtiter plate to direct sunlight. Covering the plate with e.g. aluminum foil is recommended. Return Substrate Reagent to 4°C immediately after the necessary volume is removed
13. Incubate the plate **at room temperature (ca.25°C) for 10-20 minutes, shaking at ca. 300 rpm on an orbital microplate shaker.** The incubation time may be extended up to 30 minutes if the reaction temperature is below than 20°C.
14. Add **100 µL** of **Stop Solution** to each well in the same order as the previously added Substrate Reagent.
15. Measure absorbance in each well using a spectrophotometric microplate reader at dual wavelengths of

450/540 nm. Dual wavelengths of 450/550 or 450/595 nm can also be used. Read the microplate at 450 nm if only a single wavelength can be used. Wells must be read within 30 minutes of adding the Stop Solution.

Note-1: Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels.

Note-2: Reliable standard curves are obtained when either O.D. values do not exceed 0.25 units for the blank (zero concentration), or 3.0 units for the highest standard concentration.

Note-3: If the microplate reader is not capable of reading absorbance greater than the absorbance of the highest standard, perform a second reading at 405 nm. A new standard curve, constructed using the values measured at 405 nm, is used to determine the concentration of off-scale samples. The readings at 405 nm should not replace the on-scale readings at 450 nm.

Calculations

Average the duplicate readings for each standard, control and sample, and subtract the optical density of the average zero standard. Plot the optical density versus the concentration of standards and draw the best curve. Most microtiter plate readers perform automatic calculations of analyte concentration. The standard curve fits best to a sigmoidal four-parameter logistic equation. The results of unknown samples can be calculated with any computer program having a four-parameter logistic function.

A standard curve is also to be constructed by plotting the absorbance (Y) versus log of the known concentration (X) of standards, using a cubic function. Alternatively, the logit log function can be used to linearize the standard curve (i.e. logit of optical density (Y) is plotted versus log of the known concentration (X) of standards). To determine the concentration of each sample, first find the optical density on the y-axis and extend a horizontal line to the standard curve. At the point of intersection, extend a vertical line to the x-axis and read the corresponding concentration.

If the samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.

Measurement Range

The measurement range is 15 pg/mL to 960 pg/mL. Any sample reading higher than the highest standard should be diluted with Sample Dilution Buffer in higher dilution and re-assayed. Dilution factors need to be taken into consideration in calculating the human LYPD6B concentration.

Troubleshooting

1. All samples and standards should be assayed in duplicate, using the protocol described in **Detailed Protocol**. Incubation times or temperatures significantly different from those specified may give erroneous results.
2. Poor duplicates, accompanied by elevated values for wells containing no sample, indicate insufficient washing. If all instructions in **Detailed Protocol** were followed accurately, such results indicate a need for washer maintenance.
3. Overall low signal may indicate that desiccation of the plate has occurred between the final wash and addition of Substrate Reagent. Do not allow the plate to dry out. Add Substrate Reagent immediately after wash.

Reagent Stability

All of the reagents included in the MBL Research Product **CircuLex Human LYPD6B ELISA Kit** have been tested for stability. Reagents should not be used beyond the stated expiration date.


Assay Characteristics

1. Sensitivity

The limit of detection (defined as such a concentration of human LYPD6B giving absorbance higher than mean absorbance of blank* plus three standard deviations of the absorbance of blank: A blank + 3SD blank) is better than 9.2 pg/mL of sample.

* Sample Dilution Buffer was pipetted into blank wells.

Typical standard curve

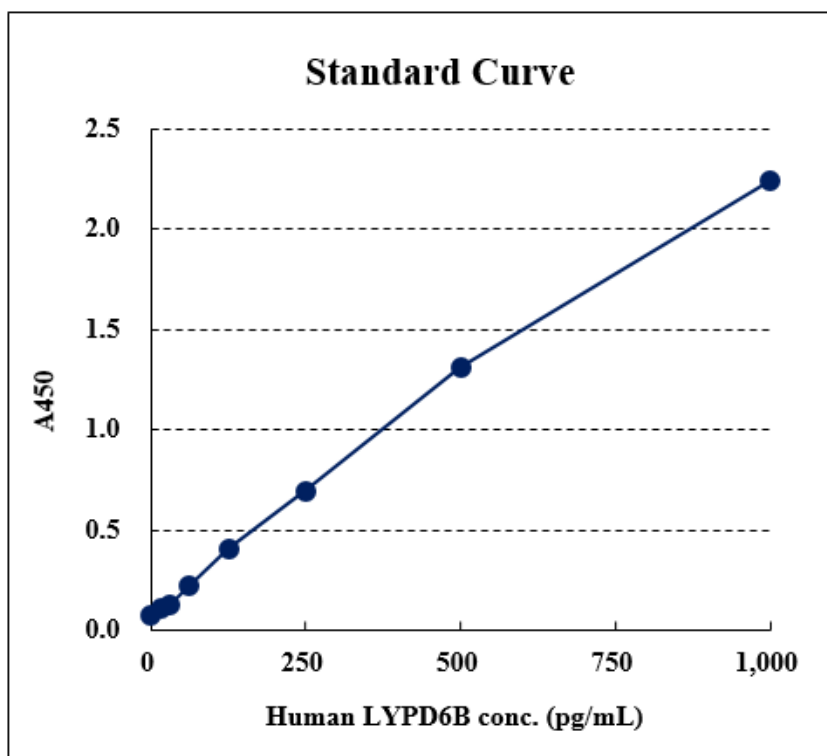

2. Precision

Intra-assay Precision (Precision within an assay)

Three samples* of known concentration were tested sixteen times on one plate to assess intra-assay precision.

- Intra-assay (Within-Run, n=16) CV=4.2, 3.8, 4.2 %

* Sample: Cell culture supernatant

Human LYPD6B conc. (pg/mL)			
	Sample 1	Sample 2	Sample 3
1	528.3	369.2	109.4
2	555.2	358.6	108.8
3	561.6	343.7	100.0
4	531.1	346.3	100.9
5	529.9	334.1	96.9
6	518.8	353.3	103.7
7	512.1	355.2	104.1
8	533.2	369.5	113.6
9	522.0	395.0	102.3
10	508.6	357.3	102.7
11	500.5	368.5	97.9
12	530.8	359.2	101.2
13	516.2	357.9	100.3
14	490.1	355.8	103.1
15	481.8	368.0	104.0
16	500.2	349.9	103.3
MAX.	561.6	395.0	113.6
MIN.	481.8	334.1	96.9
MEAN	520.0	358.9	103.3
S.D.	21.4	13.8	4.3
C.V.	4.1%	3.8%	4.2%

Inter-assay Precision (Precision between assays)

Three samples* of known concentration were tested in five separate assays to assess inter-assay precision.

- Inter-assay (Run-to-Run, n=5) CV=4.3, 6.4, 7.2 %


* Sample: Cell culture supernatant

	Human LYPD6B conc. (pg/mL)		
	Sample 1	Sample 2	Sample 3
1	409.8	325.3	81.0
2	452.0	352.4	93.6
3	410.3	304.4	81.5
4	412.3	343.1	84.2
5	420.3	308.6	77.7
MAX.	452.0	352.4	93.6
MIN.	409.8	304.4	77.7
MEAN	420.9	326.8	83.6
S.D.	17.9	21.0	6.1
C.V.	4.3%	6.4%	7.2%

3. Linearity

To assess the linearity of the assay, three samples* were serially diluted with Sample Dilution Buffer to produce samples with values within the dynamic range of the assay.

* Sample: Cell culture supernatant

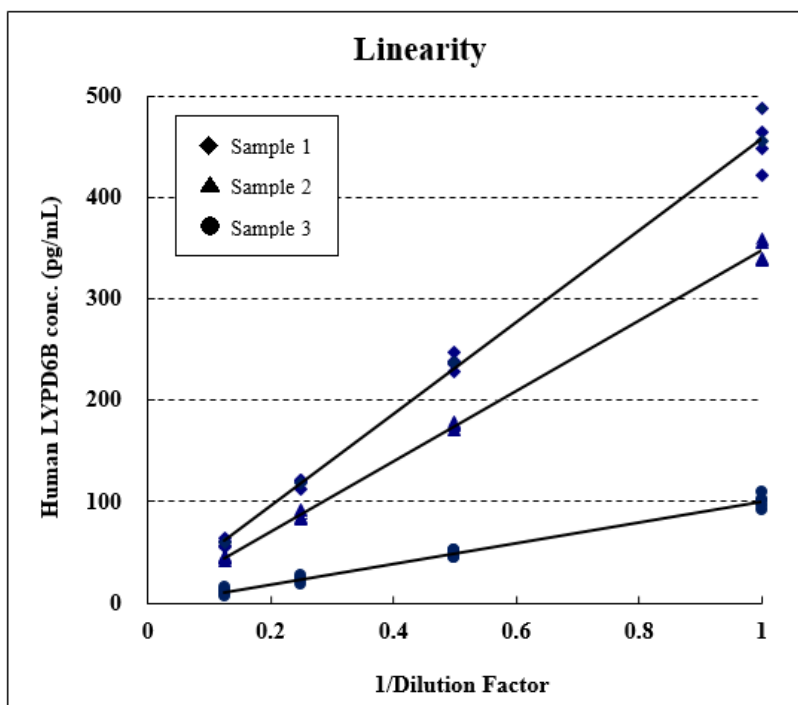

Example of Test Results

Fig.1 Human LYPD6B concentration in healthy volunteers' sera (n=24)


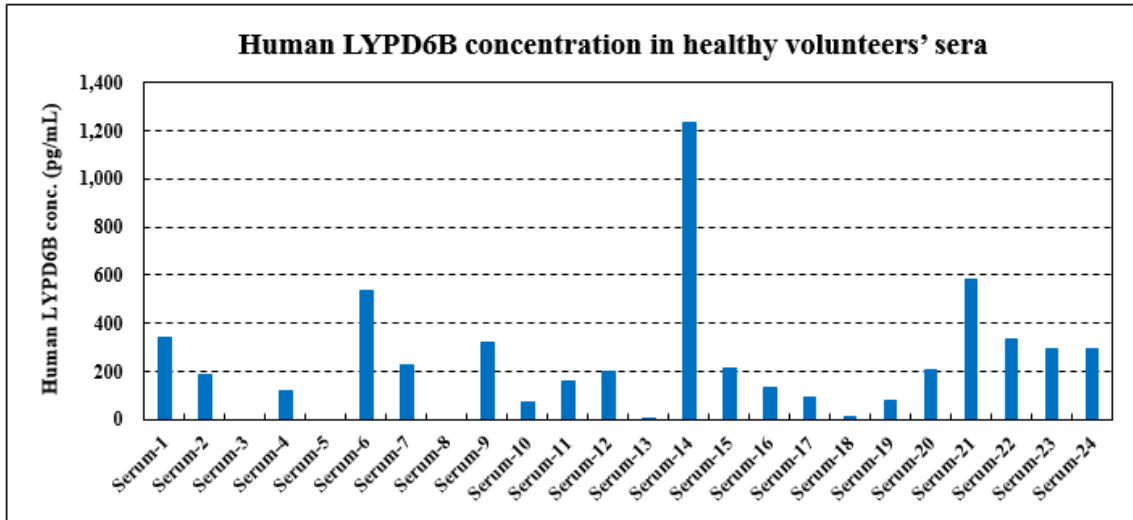


Fig.2 Human LYPD6B concentration in cell culture supernatants

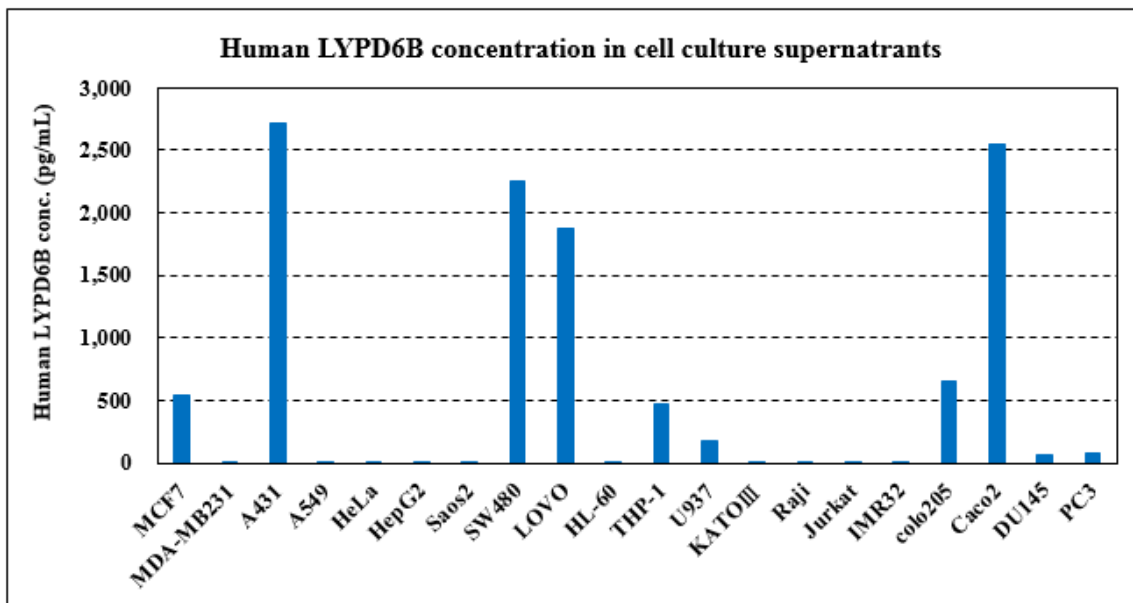

References

1. Ni J *et al.* Cloning and characterization of a human LYPD7, a new member of the Ly-6 superfamily. *Mol Biol Rep.* 2009 Apr;36(4):697-703.
2. Hillier LW *et al.* Generation and annotation of the DNA sequences of human chromosomes 2 and 4. *Nature.* 2005 Apr 7;434(7034):724-31.
3. Mallya M *et al.* Characterization of the five novel Ly-6 superfamily members encoded in the MHC, and detection of cells expressing their potential ligands. *Protein Sci.* 2006 Oct;15(10):2244-56.
4. Lee PY *et al.* Ly6 family proteins in neutrophil biology. *J Leukoc Biol.* 2013 Oct;94(4):585-94.

Related Products

- * CircuLex Human FAM3D ELISA Kit: Cat# CY-8201
- * CircuLex Human MICA ELISA Kit: Cat# CY-8206
- * CircuLex Human MICB ELISA Kit: Cat# CY-8207
- * CircuLex Human LYPD6B ELISA Kit: Cat# CY-8212
- * CircuLex Human REG4 ELISA Kit: Cat# CY-8213
- * CircuLex Human Elafin/SKALP ELISA Kit: Cat# CY-8214
- * CircuLex Human soluble Nectin-4 ELISA Kit: Cat# CY-8217
- * CircuLex Human soluble Tie-1 ELISA Kit: Cat# CY-8218
- * CircuLex Human Amphiregulin/AREG ELISA Kit: Cat# CY-8220
- * CircuLex Human TGF α ELISA Kit: Cat# CY-8221
- * CircuLex Human soluble IL-6 Receptor ELISA Kit: Cat# CY-8222

MANUFACTURED BY

MBL

MEDICAL & BIOLOGICAL LABORATORIES CO., LTD.

URL: <http://ruo.mbl.co.jp>

E-mail: support@mbi.co.jp

TEL: +81-52-238-1904

CycLex/CircuLex products are supplied for research use only. CycLex/CircuLex products and components thereof may not be resold, modified for resale, or used to manufacture commercial products without prior written approval from MBL. To inquire about licensing for such commercial use, please contact us via email.